




No.1 & GROWING  
**NARANG MEDICAL LIMITED**  
ISO 9001:2000, ISO 13485:2003, CE & WHO:GMP Compliance

HIP PROSTHESIS

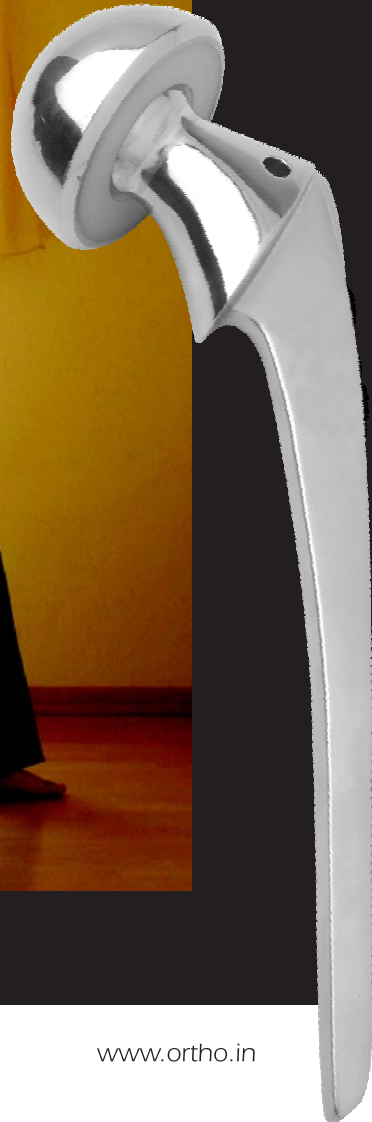

[www.ortho.in](http://www.ortho.in)




AUSTIN MOORE STEP BALL

Dia. mm	Non-Sterile Code No.	*Sterile Code No.
37	173.437	173.537
38	173.438	173.538
39	173.439	173.539
40	173.440	173.540
41	173.441	173.541
42	173.442	173.542
43	173.443	173.543
44	173.444	173.544
45	173.445	173.545
46	173.446	173.546
47	173.447	173.547
48	173.448	173.548
49	173.449	173.549
50	173.450	173.550
51	173.451	173.551
52	173.452	173.552
53	173.453	173.553
54	173.454	173.554
55	173.455	173.555
56	173.456	173.556
57	173.457	173.557

\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.

10  
2

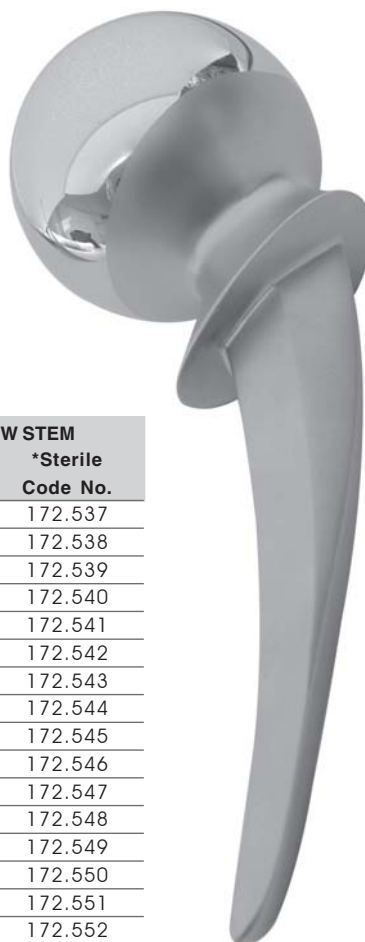

**THOMPSON HIP PROSTHESIS - EXCEL  
STAINLESS STEEL**

STANDARD STEM			NARROW STEM	
Non-Sterile	*Sterile		Non-Sterile	*Sterile
Code No.	Code No.	Dia.	Code No.	Code No.
172.037	172.237	37 mm	172.437	172.537
172.038	172.238	38 mm	172.438	172.538
172.039	172.239	39 mm	172.439	172.539
172.040	172.240	40 mm	172.440	172.540
172.041	172.241	41 mm	172.441	172.541
172.042	172.242	42 mm	172.442	172.542
172.043	172.243	43 mm	172.443	172.543
172.044	172.244	44 mm	172.444	172.544
172.045	172.245	45 mm	172.445	172.545
172.046	172.246	46 mm	172.446	172.546
172.047	172.247	47 mm	172.447	172.547
172.048	172.248	48 mm	172.448	172.548
172.049	172.249	49 mm	172.449	172.549
172.050	172.250	50 mm	172.450	172.550
172.051	172.251	51 mm	172.451	172.551
172.052	172.252	52 mm	172.452	172.552
172.053	172.253	53 mm	172.453	172.553
172.054	172.254	54 mm	172.454	172.554
172.055	172.255	55 mm	172.455	172.555

10  
3

\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.





**AUSTIN MOORE HIP  
PROSTHESIS - EXCEL  
STAINLESS STEEL (STANDARD STEM)**

<b>Dia. mm</b>	<b>Non-Sterile Code No.</b>	<b>*Sterile Code No.</b>
37	173.037	173.137
38	173.038	173.138
39	173.039	173.139
40	173.040	173.140
41	173.041	173.141
42	173.042	173.142
43	173.043	173.143
44	173.044	173.144
45	173.045	173.145
46	173.046	173.146
47	173.047	173.147
48	173.048	173.148
49	173.049	173.149
50	173.050	173.150
51	173.051	173.151
52	173.052	173.152
53	173.053	173.153
54	173.054	173.154
55	173.055	173.155
56	173.056	173.156
57	173.057	173.157
58	173.058	173.158



\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.

10  
4



**AUSTIN MOORE HIP  
PROSTHESIS - EXCEL  
STAINLESS STEEL (NARROW STEM)**

<b>Dia. mm</b>	<b>Non-Sterile Code No.</b>	<b>*Sterile Code No.</b>
37	174.037	174.237
38	174.038	174.238
39	174.039	174.239
40	174.040	174.240
41	174.041	174.241
42	174.042	174.242
43	174.043	174.243
44	174.044	174.244
45	174.045	174.245
46	174.046	174.246
47	174.047	174.247
48	174.048	174.248
49	174.049	174.249
50	174.050	174.250
51	174.051	174.251
52	174.052	174.252
53	174.053	174.253
54	174.054	174.254
55	174.055	174.255
56	174.056	174.256
57	174.057	174.257
58	174.058	174.258

\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.



10  
5





**AUSTIN MOORE HIP  
PROSTHESIS - EXCEL  
STAINLESS STEEL (BROAD STEM)**

<b>Dia. mm</b>	<b>Non-Sterile Code No.</b>	<b>*Sterile Code No.</b>
37	173.267	173.367
38	173.268	173.368
39	173.269	173.369
40	173.270	173.370
41	173.271	173.371
42	173.272	173.372
43	173.273	173.373
44	173.274	173.374
45	173.275	173.375
46	173.276	173.376
47	173.277	173.377
48	173.278	173.378
49	173.279	173.379
50	173.280	173.380
51	173.281	173.381
52	173.282	173.382
53	173.283	173.383
54	173.284	173.384
55	173.285	173.385
56	173.286	173.386
57	173.287	173.387
58	173.288	173.388



10  
6

\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.



**AUSTIN MOORE HIP PROSTHESIS  
EXTRA LONG STEM  
STAINLESS STEEL**

<b>Dia. mm</b>	<b>Non-Sterile Code No.</b>	<b>*Sterile Code No.</b>
37	175.037	175.137
38	175.038	175.138
39	175.039	175.139
40	175.040	175.140
41	175.041	175.141
42	175.042	175.142
43	175.043	175.143
44	175.044	175.144
45	175.045	175.145
46	175.046	175.146
47	175.047	175.147
48	175.048	175.148
49	175.049	175.149
50	175.050	175.150
51	175.051	175.151
52	175.052	175.152
53	175.053	175.153
54	175.054	175.154
55	175.055	175.155

Stem Length: 300mm

\*Minimum Order for Assorted Sizes for Sterile Items are: 100 Pcs.

10  
7





**BIPOLAR HIP PROSTHESIS  
STAINLESS STEEL**

<b>Dia. mm</b>	<b>*Sterile Code No.</b>
37	175.237
38	175.238
39	175.239
40	175.240
41	175.241
42	175.242
43	175.243
44	175.244
45	175.245
46	175.246
47	175.247
48	175.248
49	175.249
50	175.250
51	175.251
52	175.252
53	175.253
54	175.254
55	175.255

\*Minimum Order for  
Assorted Sizes for Sterile  
Items are: 100 Pcs.

10  
8



□ INSTRUMENTS FOR FEMORAL HEAD



**Rasp for Austin Moore**  
Code No.: 386.010



**Rasp for Austin Moore Extra Long**  
Code No.: 386.011



**Rasp for Thomposon**  
Code No.: 386.020



**Rasp for Bipolar**  
Code No.: 175.261



**Moore Hollow Chisel**  
Code No.: 386.040






**INSTRUMENTS FOR FEMORAL HEAD**



**Murphy Lane Bone Skid**  
Code No.: 386.030

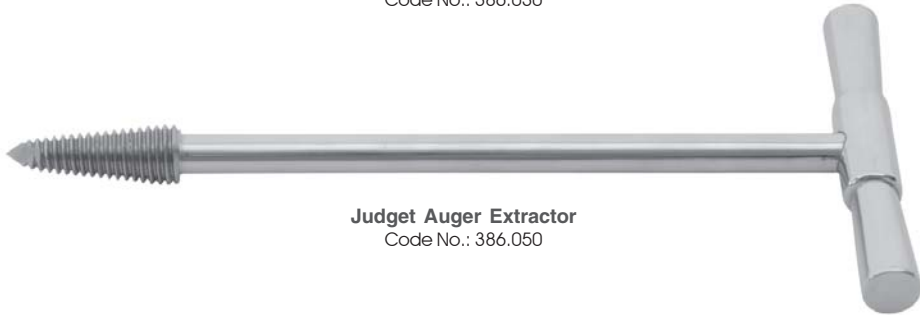

**Judet Auger Extractor**  
Code No.: 386.050



**Extractor Set for A.M. Prosthesis with 2 Hooks**  
Code No.: 386.080



**Spare Hook for A.M. Extractor**  
Code No.: 386.090



**Measuring Gauge for Prosthesis**  
Code No.: 386.060



**Impactor Nylon Faced**  
Code No.: 386.070

10  
10